



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification ⁶ : A61B 5/00</p>	<p>A1</p>	<p>(11) International Publication Number: WO 98/55016</p> <p>(43) International Publication Date: 10 December 1998 (10.12.98)</p>
<p>(21) International Application Number: PCT/US98/10864</p> <p>(22) International Filing Date: 28 May 1998 (28.05.98)</p> <p>(30) Priority Data: 1006254 6 June 1997 (06.06.97) NL</p> <p>(71) Applicant (for all designated States except US): CORDIS CORPORATION [US/US]; 14201 N.W. 6th Avenue, Miami Lakes, FL 33014 (US).</p> <p>(71)(72) Applicants and Inventors: HURTAK, Wenzel, Franz [NL/NL]; Aan De Vaart 10, NL-9301 TZ Roden (NL). MOUS, Frans [NL/NL]; Ploeggang 6, NL-9203 HP Drachten (NL). NAP, Cornelis, Philipus [NL/NL]; Oude Streek 10, NL-9345 AG Zevenhuizen (NL).</p> <p>(74) Agent: MONTGOMERY, Michael, W.; 14201 N.W. 60th Avenue, Miami Lakes, FL 33014 (US).</p>		<p>(81) Designated States: AU, CA, JP, MX, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p>Published With international search report.</p>
<p>(54) Title: GLASS CORE GUIDEWIRE COMPATIBLE WITH MAGNETIC RESONANCE HAVING REINFORCING FIBERS</p> <div data-bbox="365 1207 1347 1806"> </div> <p>(57) Abstract</p> <p>A medical guidewire (1) is intended for use in intravascular medical procedures involving the use of magnetic resonance systems. The guidewire (1) has a body (2) and a distal tip portion (3). The distal tip of the guidewire (1) includes several markers (4) embedded in the distal tip portion (3), which are more visible under MR than the remainder of the guidewire.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

**GLASS CORE GUIDEWIRE COMPATIBLE WITH MAGNETIC RESONANCE
HAVING REINFORCING FIBERS**

BACKGROUND AND SUMMARY OF THE INVENTION

1. Technical Background:

The present invention relates generally to intravascular medical devices, and more particularly, to a medical guidewire having reinforcing fibers for use with magnetic resonance
5 systems. Such guidewires may be used in medical procedures for both diagnostic and interventional purposes.

2. Discussion:

Guidewires are used in a wide variety of medical procedures, most often in conjunction with one or more other medical devices, including catheters. Such a catheter may be any of
10 various types, such as angiography or angioplasty, but should in any event have a tubular lumen or other guiding means through which the guidewire can be advanced or withdrawn.

Structurally, guidewires are often long, thin metal wires that generally taper from one diameter at a proximal end which remains outside the body of the patient, to a smaller diameter at the opposite distal end. Specifically, vascular guidewires are often more than five feet long
15 and have a maximum outer diameter of approximately 0.035 inches. The diameter of the core wire is generally ground down precisely in a series of alternating tapering portions and constant diameter sections, to develop a selectively engineered flexibility profile along the length of the guidewire.

The guidewire distal tip is usually very flexible, both to avoid vascular trauma and so that it can be selectively bent and twisted to advance it along a desired vascular path. Guidewires are designed to resist this twisting force or torsion, so that as the guidewire proximal end is twisted or rotated, the distal tip tends to rotate through about the same angle.

5 In addition, a floppy spring is often affixed to the extreme distal tip of the guidewire for flexibility.

A good example of a current guidewire is described in the commonly assigned United States Patent number 4,846,186, issued to Box et al. on July 11, 1989, which is incorporated in this disclosure by reference. The Box patent shows a guidewire suitable for both
10 diagnostic and therapeutic or interventional procedures, having a Teflon coating from the proximal end along a majority of its length. The core wire tapers in steps to a distal portion that is flattened and surrounded by a flexible spring, which is brazed to the extreme distal end of the core wire to form a rounded tip.

As the body of the patient is of course opaque, physicians commonly use fluoroscopy
15 or X-ray video cameras to track the position of the guidewire and to construct real-time images of the patient's vasculature. The visibility and brightness of selected portions of the guidewire is a relatively important feature, as described in the commonly assigned United States Patent number 5,259,393, issued to Corso, Jr. et al. on November 9, 1993, and United States Patent number 5,267,574, issued to Viera et al. on December 7, 1993. Both of these
20 patents are incorporated in this disclosure by reference. In the Corso patent, the flexible spring at the guidewire distal tip is arranged to selectively control its brightness on an X-ray fluoroscope, or radiopacity. Likewise, the Viera patent discloses a plastic sleeve shrunk around an intermediate section of the guidewire, and several radiopaque marker bands.

In contrast to fluoroscopy, another method of visualizing the patient is magnetic resonance imaging, referred to as MRI. Other medical fields, such as neurology, often use procedures which are performed under MRI instead of X-ray fluoroscopy. Accordingly, it is also desirable to image the anatomy and to track the position of intravascular devices, including catheters and guidewires, using magnetic resonance (MR) systems.

For these applications, it is desirable to make guidewires usable and compatible with MRI techniques. However, a metal guidewire may be too visible under MR, brightly washing out the screen and obscuring important features. This halo phenomenon is called an "artifact," and renders the image useless. Another issue with the use of a metal guidewire under MR is the induction of eddy currents in the metal, caused by distortion of the magnetic field. These eddy currents can generate heat and may increase the local temperature of the surrounding tissue and body fluids, thus possibly damaging the tissue or causing the blood to coagulate.

It is an object of the present invention to provide a guidewire having the desired physical features, including torsion and flexibility, while also avoiding the creation of undesirable artifacts in the MR image or the generation of heat.

The present invention provides a guidewire compatible for use with magnetic resonance systems, made from a non-metallic material with a high specific electric impedance. Accordingly, this material will resist any electrical eddy currents in the guidewire from being generated by variations in the high-frequency field. An acceptable class of materials is glass, which are all electrical insulators. A guidewire having a major portion constructed of a glass material should therefore have the advantages of not disturbing the MR field and images, as well as resisting the generation of heat.

These and various other objects, advantages and features of the invention will become apparent from the following description and claims, when considered in conjunction with the appended drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

5 Figure 1 is a perspective view of a guidewire for use with magnetic resonance systems, arranged according to the present invention;

Figure 2 is a cross-sectional view of an intermediate portion of the guidewire of Figure 1;

10 Figure 3 is a cross-sectional view of a proximal end portion of the guidewire of Figure 1;

Figure 4 is a perspective view of a guidewire for use with magnetic resonance systems, arranged according the present invention;

Figures 5-7 are cross-sectional views of a portion of various guidewires arranged according to certain embodiments of the present invention;

15 Figure 8 is a perspective view of a guidewire for use with magnetic resonance systems, illustrating the reinforcing fibers of the present invention;

Figure 9 is a cross-sectional view of an intermediate portion of the guidewire of Figure 8;

20 Figure 10 is a cross-sectional view of a proximal end portion of the guidewire of Figure 8; and

Figures 11-13 are side elevation views of distal portions of guidewires arranged according to alternative embodiments of the present invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

The following description of the preferred embodiments of the present invention is merely illustrative in nature, and as such it does not limit in any way the present invention, its application, or uses. Numerous modifications may be made by those skilled in the art without
5 departing from the true spirit and scope of the invention.

Referring to Figure 1, a perspective view of a stent according to a preferred embodiment of the present invention is shown generally at 1. The medical guidewire 1 is intended for use in intravascular medical procedures involving the use of magnetic resonance systems, including both magnetic resonance imaging and magnetic resonance tracking of the
10 guidewire's position within the body of the patient. Guidewire 1 is constructed of a basic body 2 and a distal tip portion 3. The distal tip of guidewire 1 includes several markers 4 embedded in the distal tip portion 3, which are more visible under MR than the remainder of the guidewire.

The proximal portion of the basic body 2 is illustrated in Figure 3, and incorporates a
15 relatively long, thin core or glass body 5, which may be encased with a protective coating 6. The coated glass body 5 extends for substantially the length of the guidewire and is surrounded with a polymer sheath 7, which is adhered to the glass body 5 with a glue 8.

Markers 4 are visible under MR because they are susceptible to slightly distorting the uniformity of the magnetic resonance field, causing the magnetic field to become what is
20 called "inhomogeneous." The material of the markers 4 is selected specifically for this property, and acceptable materials include Dysprosium Oxide (Dy_2O_3).

The glass body 5 is preferably made of a glass material having a high specific electric impedance, such as fiberglass, silica, or quartz.

The coating 6 adds strength to the glass core 5, in that the coating allows the glass core 5 to be bent through a sharper turn or more tortuous path without breaking. Indeed, it has been found that the coated glass core 5 may endure strain as high as 12%. A suitable material for the coating 6 has been found to be polyimide.

5 The outer polymer sheath 7 may be constructed from any of a variety of materials, including nylon. An additional advantage of the design of the present invention is that the polymer sheath 7 can maintain the physical integrity of the guidewire, even if the glass core 5 should unexpectedly break. Of course, the polymer sheath 7 may be provided with a lubricious or hydrophilic coating, as generally known in the art.

10 An intermediate portion of the guidewire is depicted in Figure 2, which focuses on a region near the transition at arrow II between the glass core proximal portion of the basic body, referred to as the "transition point."

The distal tip portion 3 of the guidewire 1 may be formed of a plastic, as shown in Figure 2, or of a metal as shown in Figures 8-13. The outer diameter of guidewire 1
15 preferably tapers to a smaller diameter toward the distal tip, as illustrated in Figures 8-13. The metal tip portion may be stainless steel or more preferably nickel titanium, or nitinol. Preferably, the length of the metal distal tip segment is substantially shorter than the wavelength of the magnetic resonance field in which the guidewire is used.

The glue 8 is preferably of a type that cures upon exposure to ultraviolet light.
20 Accordingly, the polymer sheath 7 should be transparent, to allow the glue 8 to be exposed to the ultraviolet light after portions of the guidewire 1 are assembled as shown in Figures 1-3.

An embodiment of the present invention is depicted in Figures 4-7, in which a guidewire 11 has a proximal portion 12 and a distal tip portion 13. Guidewire 11 has a plastic sheath 16 in which a number of reinforcing fibers have been embedded. Sheath 16 may be shrunk around a bundle of fibers 17, or the sheath 16 may be braided with the reinforcing fibers. Alternatively, fibers 18 may be embedded in a polymer matrix 19. In addition, a multiplicity of short reinforcing fibers 20 can be provided in a polymer matrix 21, surrounded by a coating 12. Accordingly, the present invention includes the provision of reinforcing fibers in either the core of the guidewire or the plastic sheath surrounding the core. The reinforcing fibers may be of any suitable material, such as carbon, borium, aramide, or glass.

The guidewire of the present invention may also be constructed of more than one glass core body, all of which may be clad as a unit with a single protective coating.

It should be understood that an unlimited number of configurations for the present invention can be realized. The foregoing discussion describes merely exemplary embodiments illustrating the principles of the present invention, the scope of which is recited in the following claims. Those skilled in the art will readily recognize from the description, claims, and drawings that numerous changes and modifications can be made without departing from the spirit and scope of the invention.

CLAIMS

What is claimed is:

1. A medical guidewire for use in intravascular medical procedures and compatible with magnetic resonance, the guidewire having proximal and distal ends, comprising:
 - 5 a relatively long, thin core extending for substantially the length of the guidewire, the core being made of a glass having a high specific electric impedance;
 - a polymer sheath surrounding the core;
 - a plurality of reinforcing fibers affixed to at least one of the core and the polymer sheath, to enhance the flexibility and torsion characteristics of the guidewire; and
 - 10 at least one marker positioned near a distal end of the guidewire, wherein the marker is visible under magnetic resonance due to susceptibility-induced magnetic field inhomogeneity.
2. The medical guidewire of Claim 1, further comprising a relatively short distal tip
15 segment made of metal components affixed to the glass core at a transition point, wherein the length of the metal distal tip segment is substantially shorter than the wavelength of a magnetic resonance field.
3. The magnetic guidewire of Claim 1, wherein the reinforcing fibers are affixed to
20 the core.
4. The magnetic guidewire of Claim 1, wherein the reinforcing fibers are affixed to the polymer sheath.

5. The magnetic guidewire of Claim 4, wherein the material of the reinforcing fibers is selected from the group consisting of carbon, borium, aramide, and glass.

5 6. The magnetic guidewire of Claim 1, wherein the material of the core is selected from the group consisting of fiberglass, silica, and quartz.

7. The magnetic guidewire of Claim 2, wherein the material of the metal distal tip segment is nitinol.

10

8. The magnetic guidewire of Claim 1, wherein a distal segment of the glass core tapers to a diameter at the distal end of the guidewire that is smaller than the diameter of a major portion of the core.




15 9. The magnetic guidewire of Claim 2, wherein the polymer sheath extends continuously from a location near the proximal end of the guidewire, to a location distal of the transition point, thus surrounding at least a portion of both the glass core and the metal distal tip segment.

20 10. The magnetic guidewire of Claim 1, further comprising a short metal collar affixed to the guidewire at the transition point, to resist kinking and breakage of the guidewire at the transition point.

11. The magnetic guidewire of Claim 1, wherein the material of the marker is Dysprosium Oxide (Dy_2O_3).

12. The magnetic guidewire of Claim 1, wherein the distal tip of the guidewire is bent
5 slightly, to facilitate the selective steering of the guidewire along a desired vascular path.

1/3

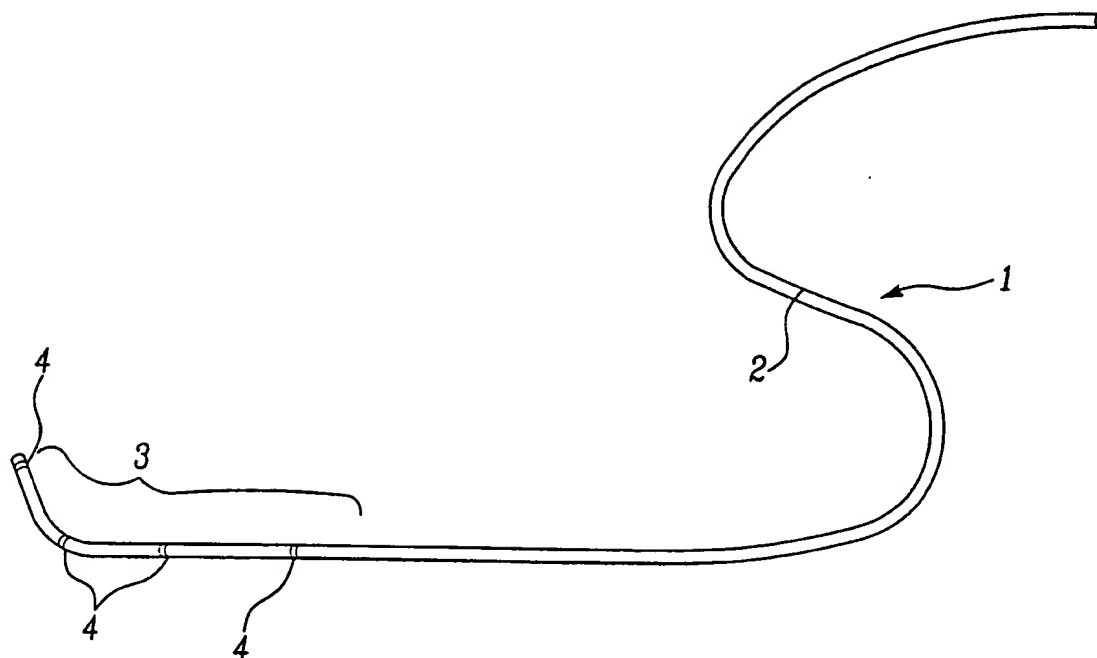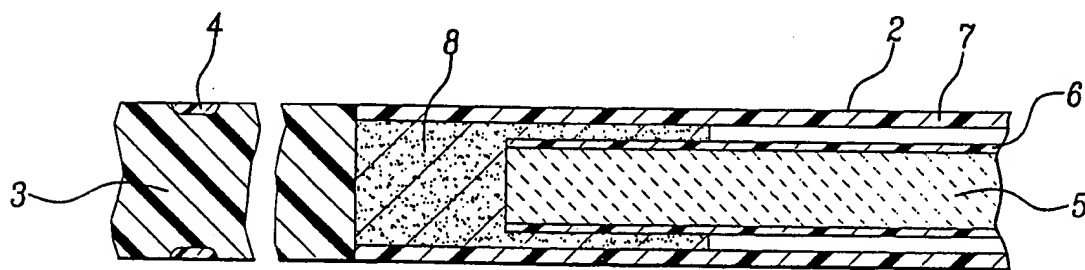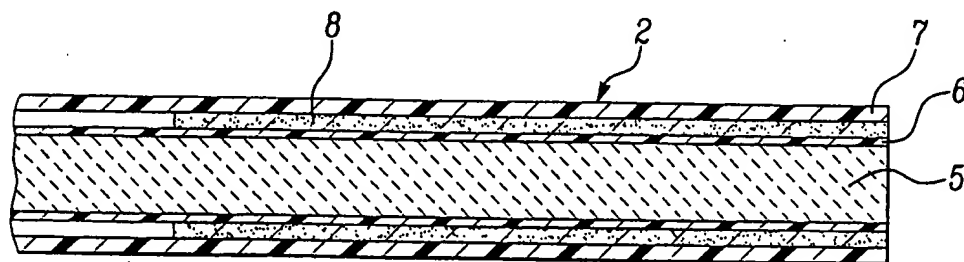Fig-1Fig-2Fig-3

2/3

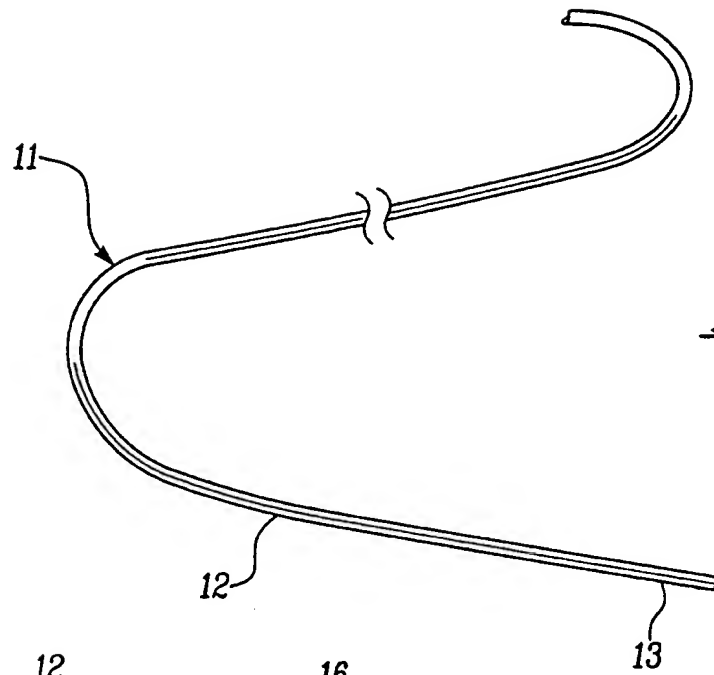


Fig-4

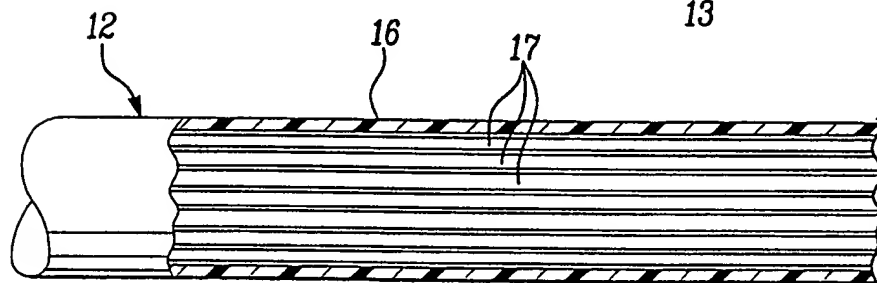


Fig-5

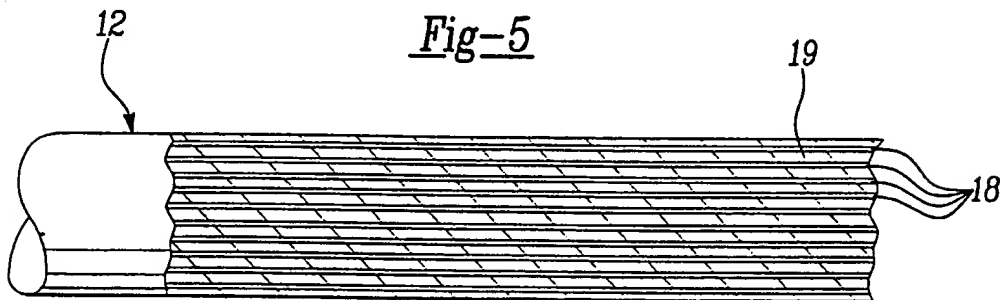


Fig-6

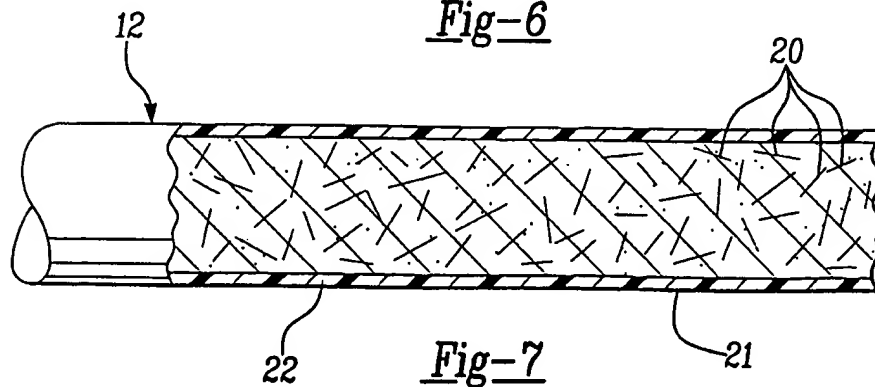


Fig-7

3/3



Fig-8

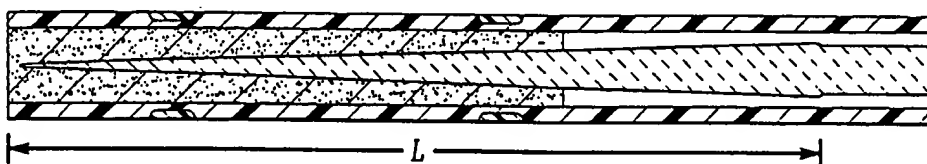


Fig-8

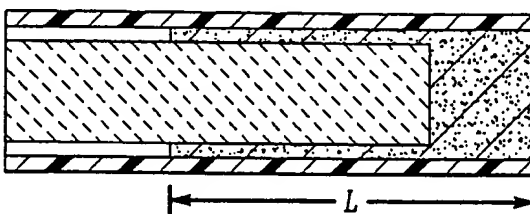


Fig-10




Fig-11




Fig-12


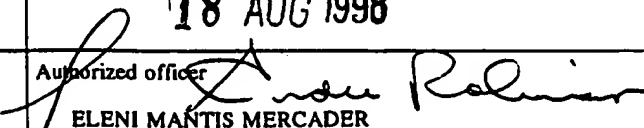


Fig-13

INTERNATIONAL SEARCH REPORT

international application No.
PCT/US98/10864

A. CLASSIFICATION OF SUBJECT MATTER IPC(6) : A61B 5/00 US CL : 600/434 According to International Patent Classification (IPC) or to both national classification and IPC														
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) U.S. : 128/899; 600/407, 410, 434, 585; 604/264, 280 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)														
C. DOCUMENTS CONSIDERED TO BE RELEVANT														
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.												
A	US 5,353,808 A (VIERA et al) 11 October 1994, entire document.	1-12												
A, P	US 5,706,827 A (EHR et al) 13 January 1998, entire document.	1-12												
A, P	US 5,769,796 A (PALERMO et al) 23 June 1998, entire document.	1-12												
A	US 5,078,700 A (LAMBERT et al) 7 January 1992, entire document.	1-12												
<input type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/> See patent family annex.														
<table border="0"> <tr> <td>* Special categories of cited documents:</td> <td>*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</td> </tr> <tr> <td>*A* document defining the general state of the art which is not considered to be of particular relevance</td> <td>*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</td> </tr> <tr> <td>*B* earlier document published on or after the international filing date</td> <td>*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</td> </tr> <tr> <td>*L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</td> <td>*A* document member of the same patent family</td> </tr> <tr> <td>*O* document referring to an oral disclosure, use, exhibition or other means</td> <td></td> </tr> <tr> <td>*P* document published prior to the international filing date but later than the priority date claimed</td> <td></td> </tr> </table>			* Special categories of cited documents:	*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention	*A* document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone	*B* earlier document published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art	*L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A* document member of the same patent family	*O* document referring to an oral disclosure, use, exhibition or other means		*P* document published prior to the international filing date but later than the priority date claimed	
* Special categories of cited documents:	*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention													
A document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone													
B earlier document published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art													
L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A* document member of the same patent family													
O document referring to an oral disclosure, use, exhibition or other means														
P document published prior to the international filing date but later than the priority date claimed														
Date of the actual completion of the international search 16 JULY 1998		Date of mailing of the international search report 18 AUG 1998												
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. (703) 305-3590		Authorized officer  ELENI MANTIS MERCADER Telephone No. (703) 308-0899												